

FIG. 2A

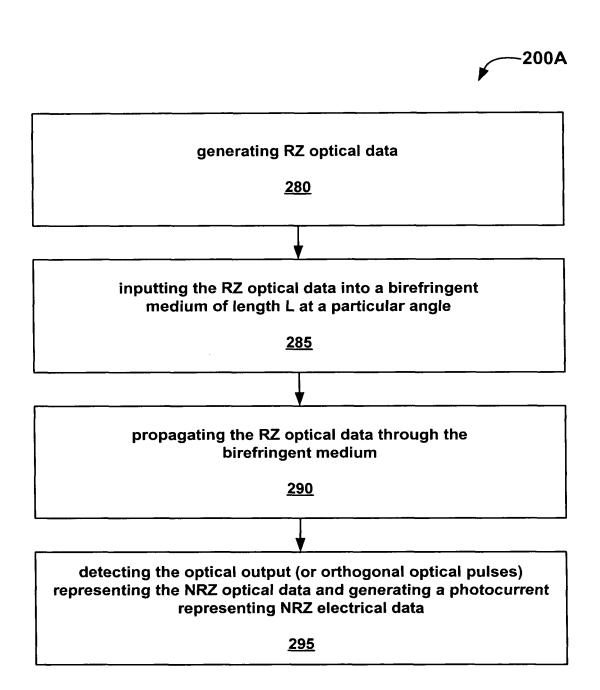


FIG. 2B



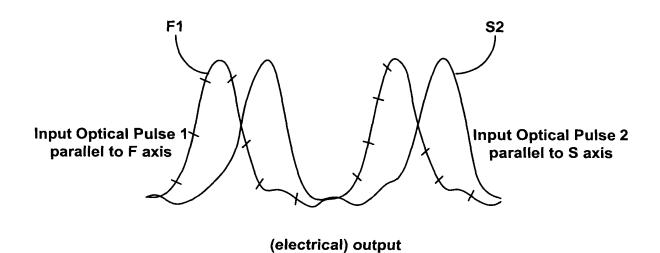


FIG. 3A


## Input Optical Pulse at 45°

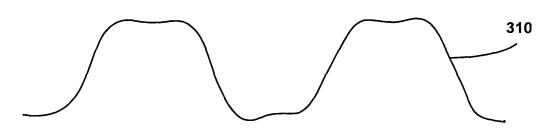

(electrical) output

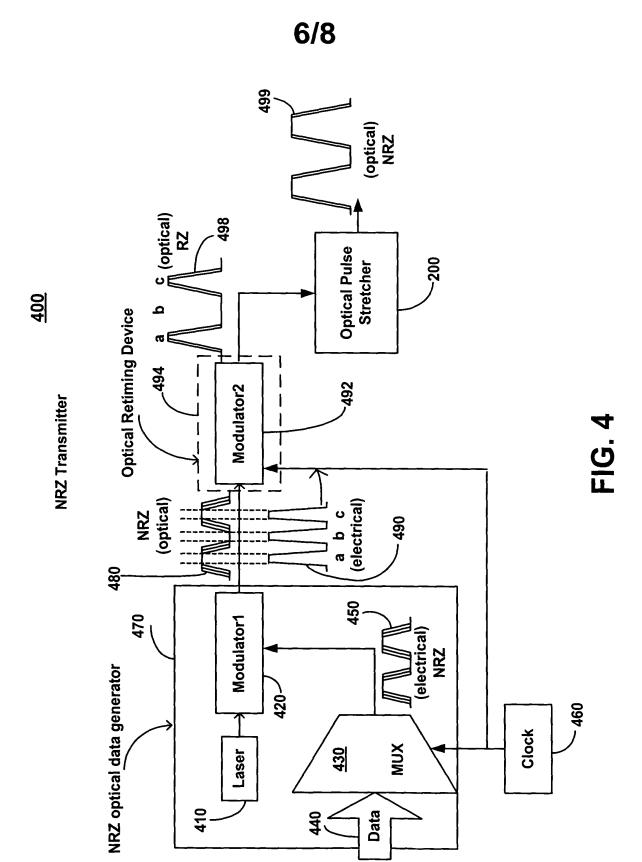

## NRZ PRBS Eye without optical retiming and without optical pulse stretcher

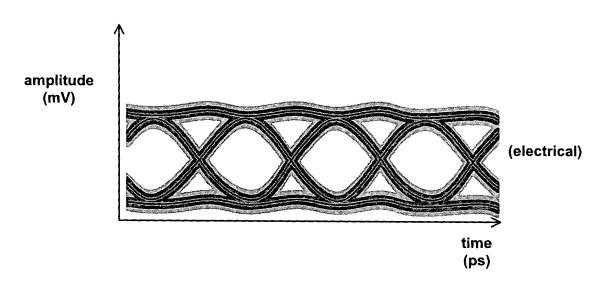

## NRZ PRBS Eye with optical retiming and with optical pulse stretcher

